



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Sirolan Laserscan Micron Test Report

Alpacas at Lone Ranch/Renate & Richard Gyuro
13856 Weowna Way
White City OR 97503-8535

06/22/16

Test No: 924749


Animal and Sample Description

Animal Name: Bellamy
Breed: Alpaca(Huacaya)
Sex: Male
Color: White

Animal ID: Pending
Sample Location: Side
Sample Date: 05/24/16
Age: 06/17/14

Laboratory Data

Mean Fiber Diameter: 19.8 microns
Standard Deviation: 4.4 microns
Coefficient of Variation: 22.4 %
Fibers Greater Than 30 microns: 1.4 %

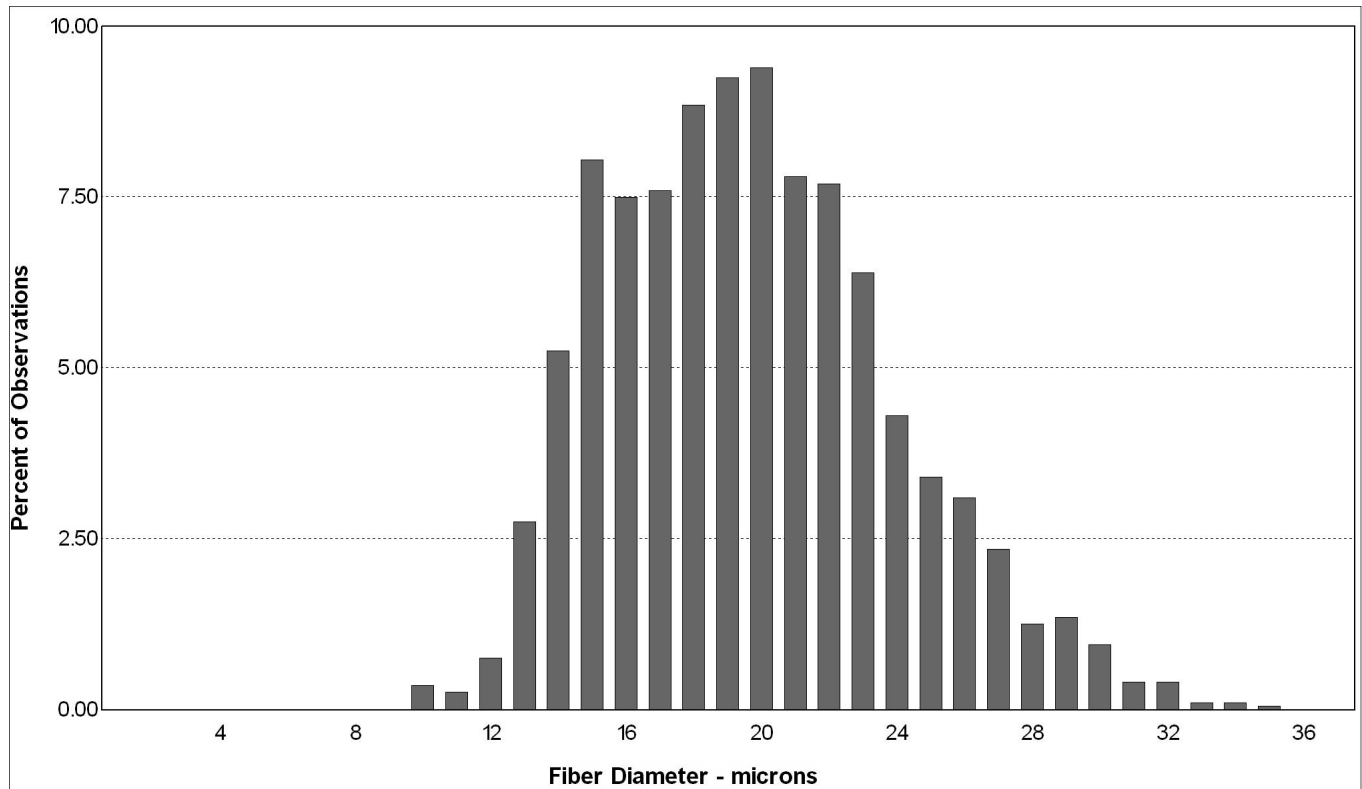

This Test Performed According to I.W.T.O Method 12